


# Confocal Microscopy and Atomic Force Microscopy (AFM) of biofilms


A very brief primer...

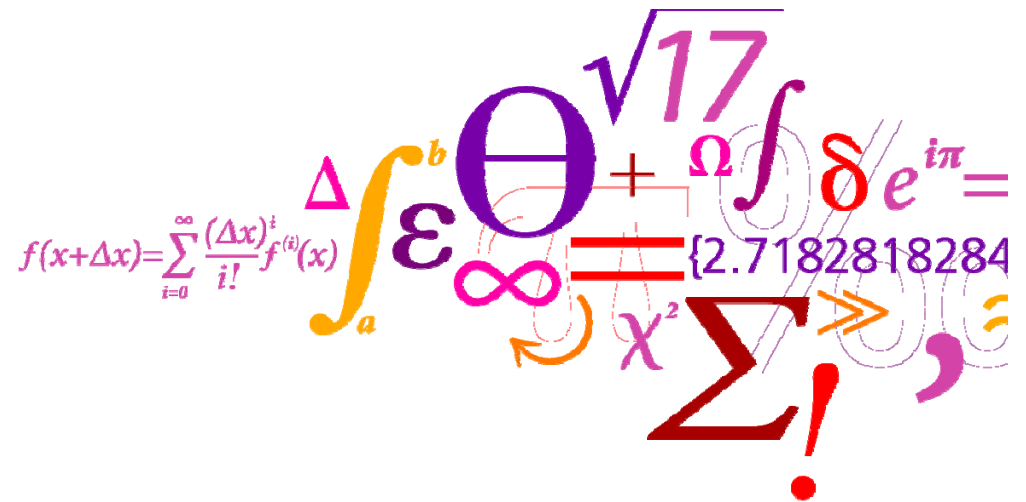


# Fundamentals of Confocal Microscopy

Based on a conventional fluorescence microscope


## Fluorescent Microscope

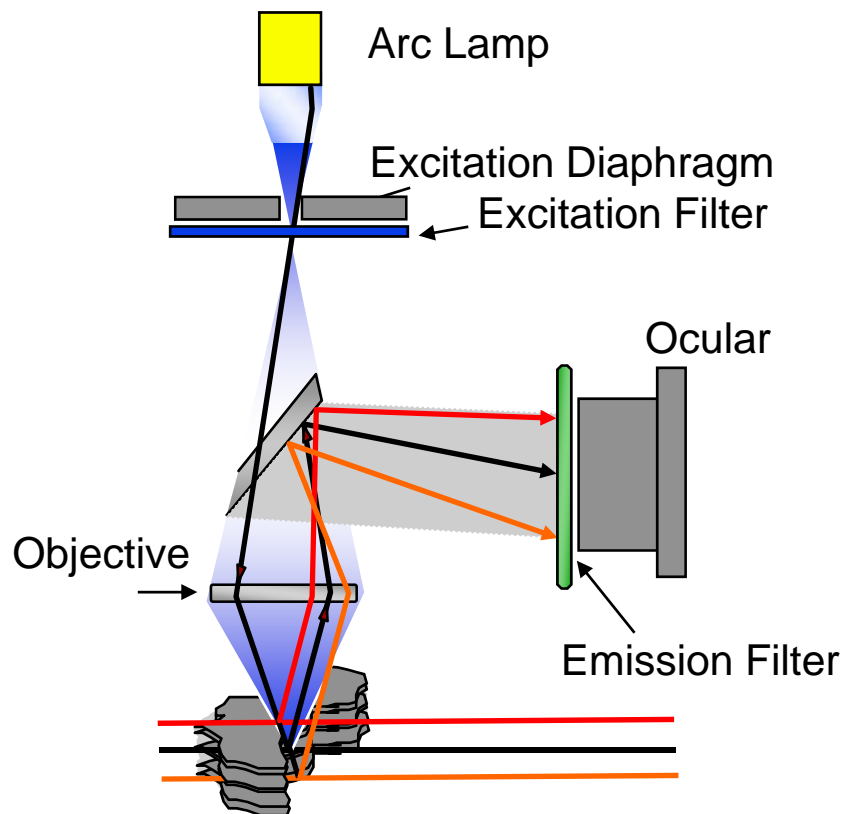


## Confocal Microscope

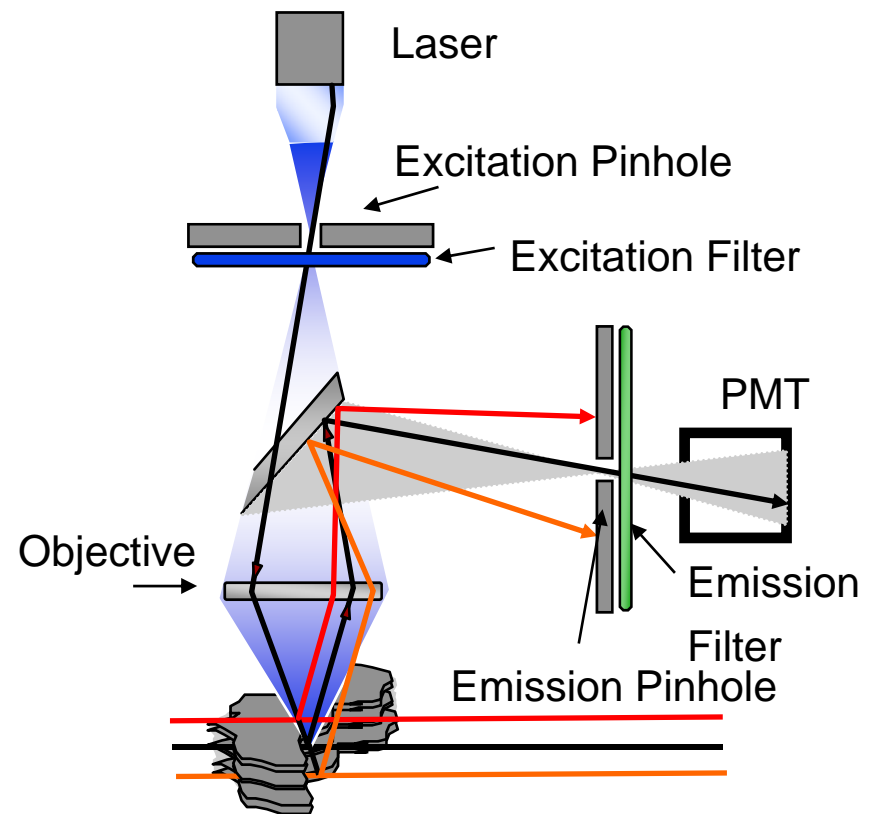

# 3D reconstruction

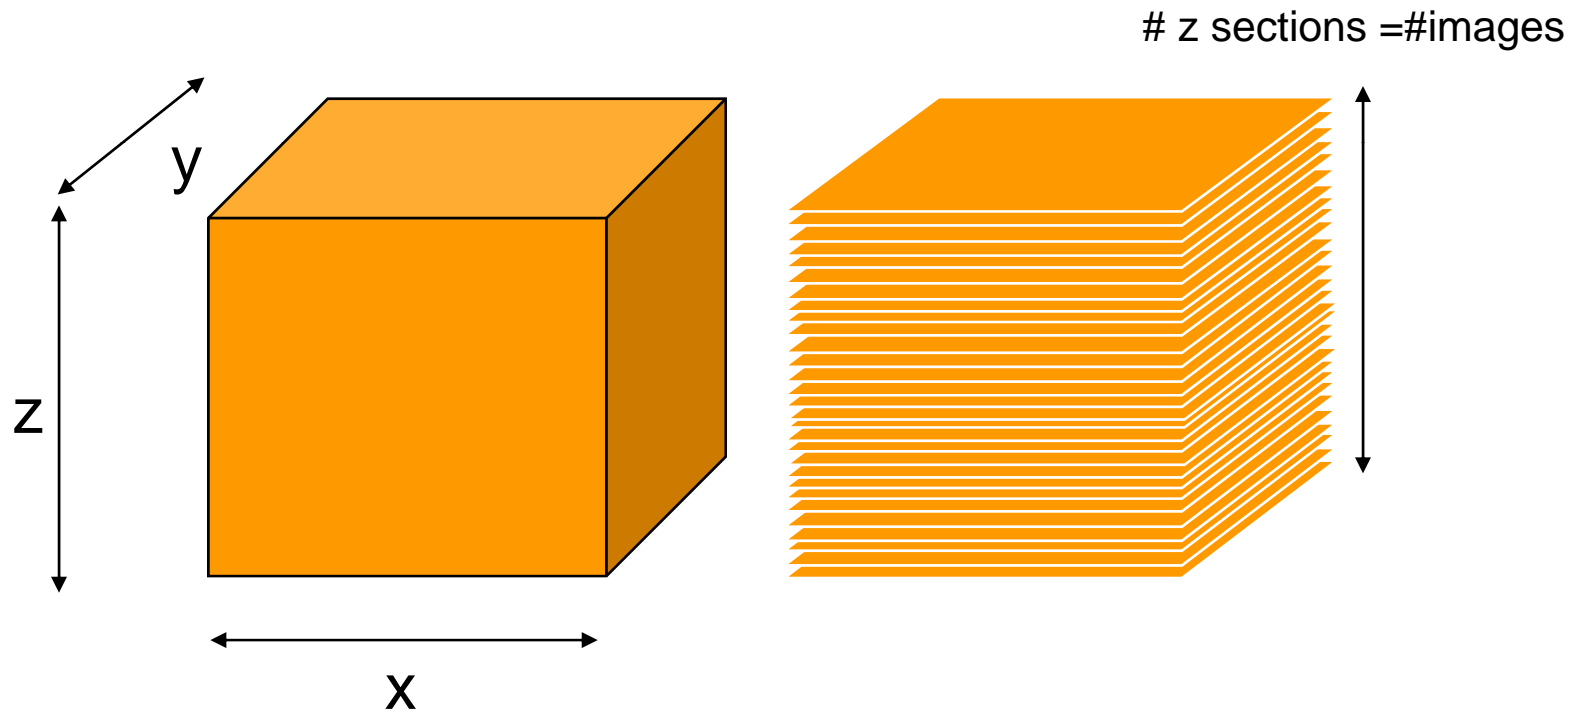

*Pseudomonas putida*  
cells mixed with  
*Acinetobacter* cells in a  
microbial biofilm

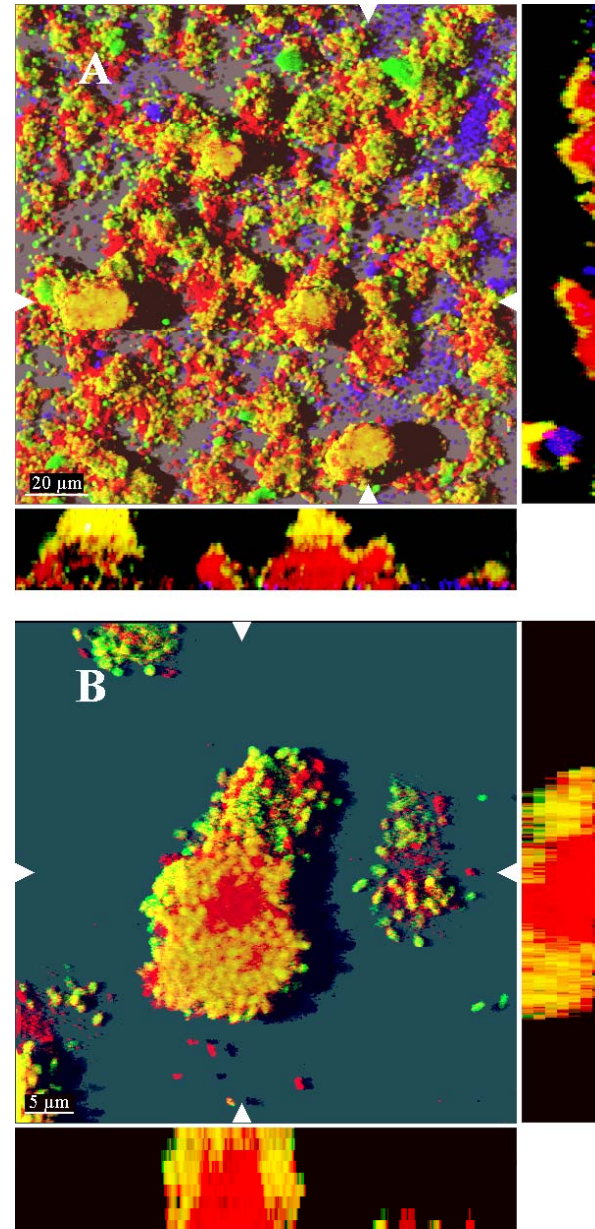


Christensen et al. 1998. Appl. Environ. Microbiol. 64: 2247-55

## Benefits of Confocal Microscopy


- Reduced blurring of the image from light scattering
- Increased effective resolution
- Improved signal to noise ratio
- Clear examination of thick specimens
- Z-axis scanning (3D-reconstruction possible)
- Magnification can be adjusted electronically
- X-Y resolution: ~200-250 nm (Ernst Abbe)

## Disadvantages of Confocal Microscopy


- Requires fluorescent samples
- Uses laser illumination (expensive, few wavelengths)
- Instrument expensive to acquire and run
- Z-resolution typically >500 nm

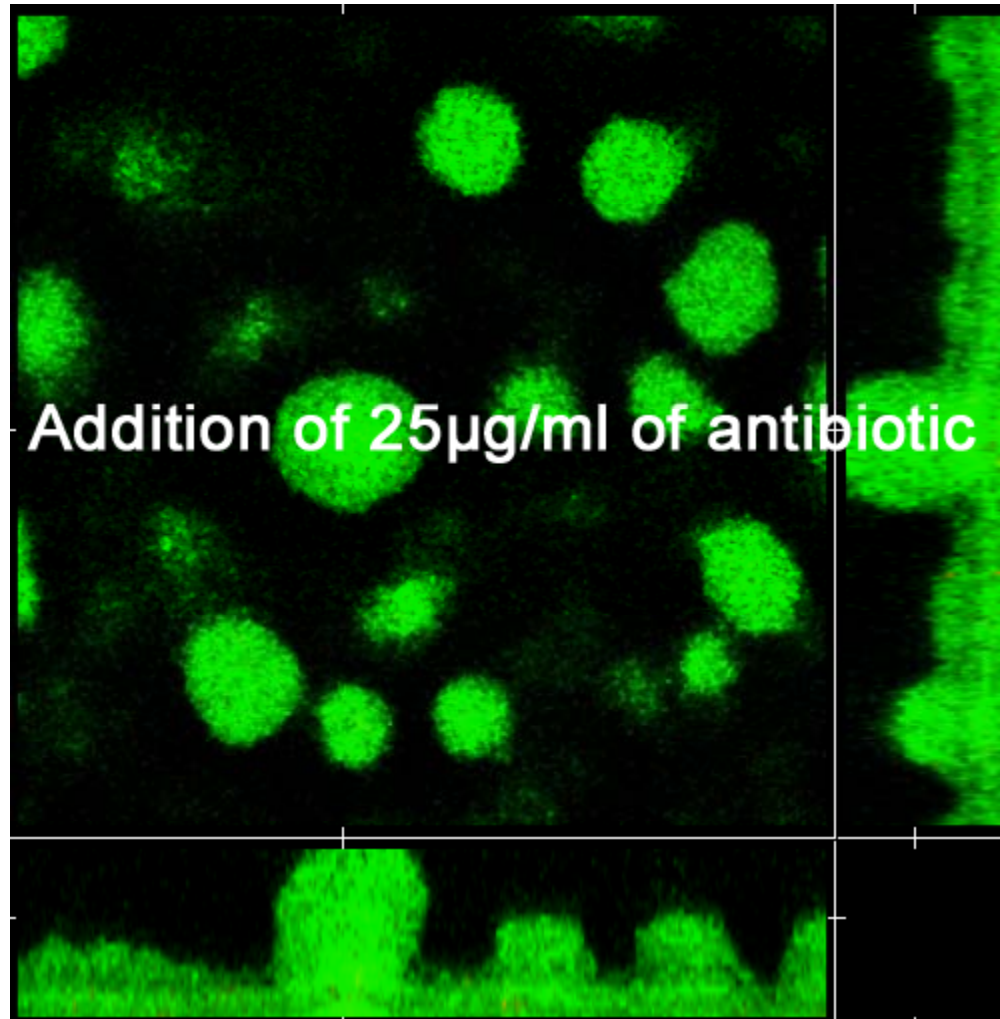

Haagensen et al. 2007. J. Bacteriol. 189:28-37

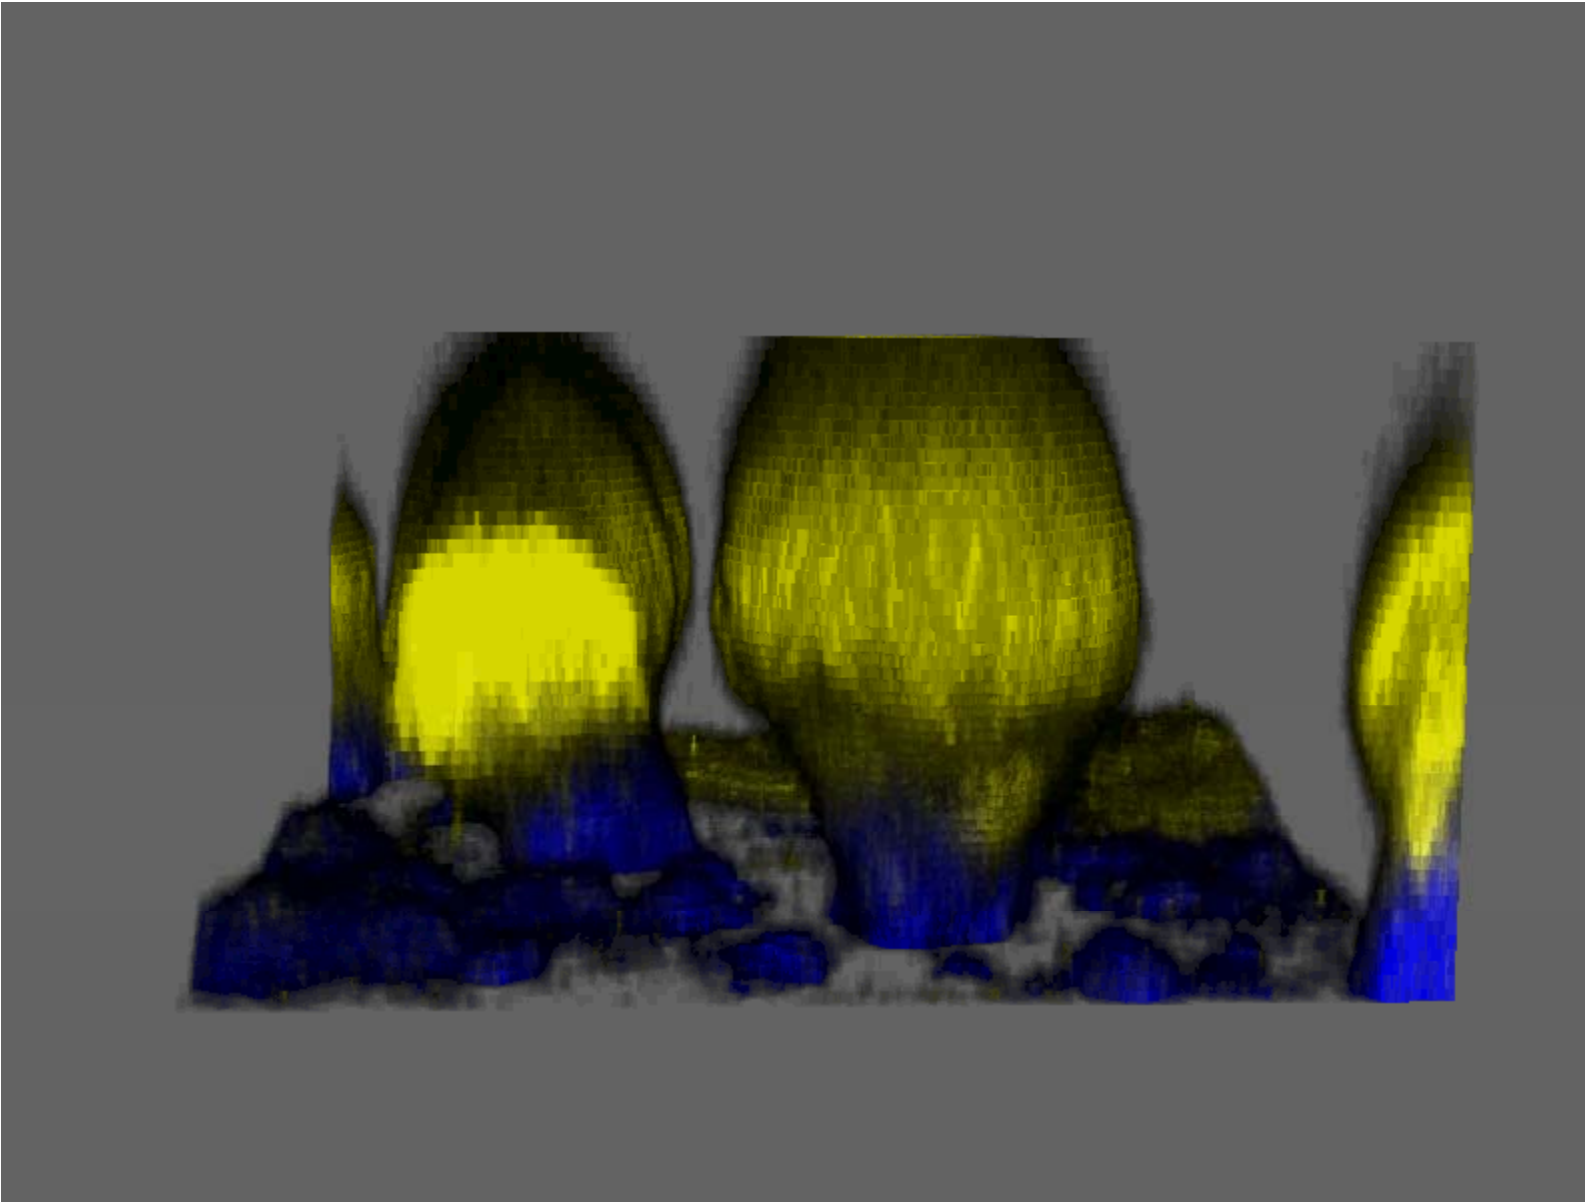

Klausen et al. 2003. Mol. Microbiol. 50: 61.68

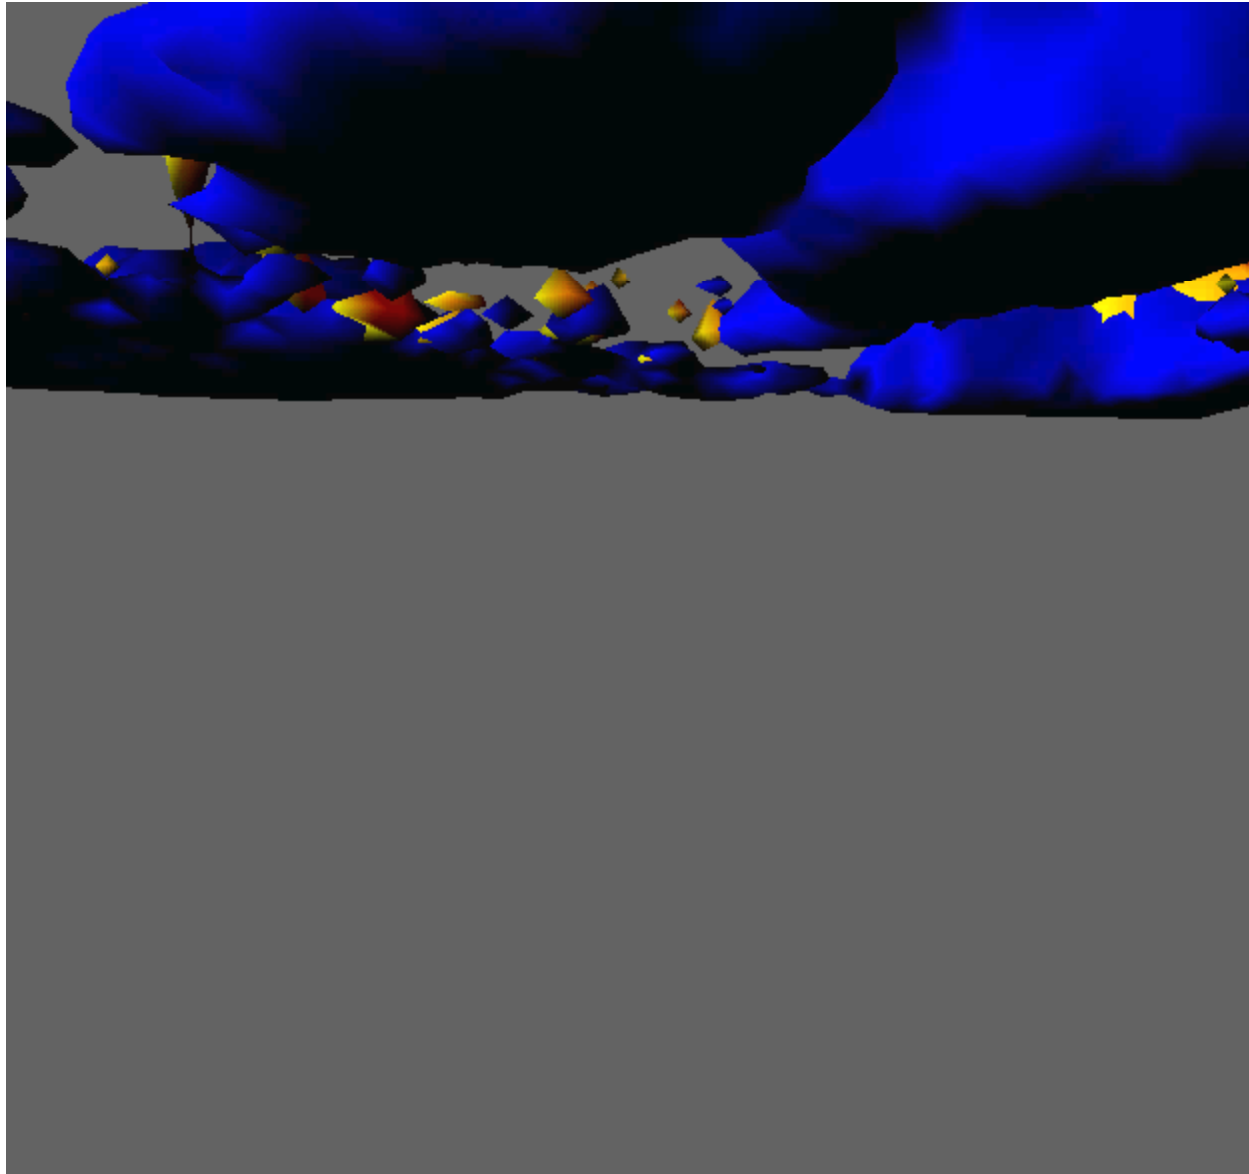




# New developments in confocal microscopy


- **MP (multi-photon) or two-photon confocal microscopy:** Two or more photons from a long wavelength illumination at a time excites a fluorophore. High resolution in Z-axis (practically down to ~200 nm)
- **White Laser (Leica):** A continuous wave "white" laser (tunable from 470-670 nm, with up to 8 lines simultaneously)
- **STED (Stimulated Emission Depletion) (Leica):** A new method where fluorescence is depleted around the area of interest (see next slide)
- **Superresolution structured microscopy (Zeiss):** A method where images are rotated and combined to create a moiré pattern which is deconvolved to create a high resolution image.
- **Photo-Activated localization microscopy (Zeiss):** Sequential illumination and localization of fluorophores combined with computational reconstruction of high resolution images.
- **Raman-confocal microscopy (Leica, under development):** Confocal microscope combined with Raman spectroscopy. Enables localized determination of [changes in] concentrations of metabolites etc.

## STED (Stimulated Emission Depletion)


- In a Leica TCS STED microscope the sample is illuminated by two pulsed laser beams, tightly synchronized.
- The 635 nm wavelength excites the fluorophores of the sample the same way a conventional confocal system does. The excitation laser pulses are directly followed by a ring shaped illumination of a Ti:Sapphire Infrared laser (730-780 nm).
- This pulse inhibits/depletes the fluorescence in the outer regions of the illuminated spot.
- The result: A smaller fluorescence spot that allows much more accurate scanning than with other methods using focused light. X-Y res: <90 nm

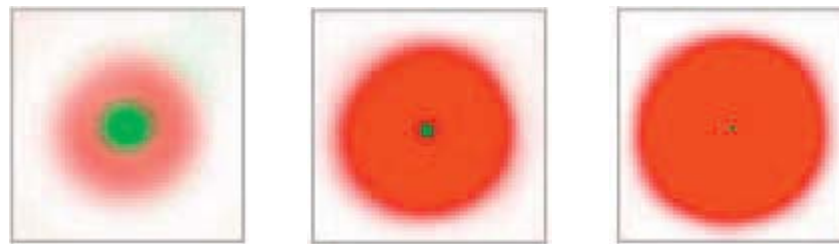

## Sample STED image

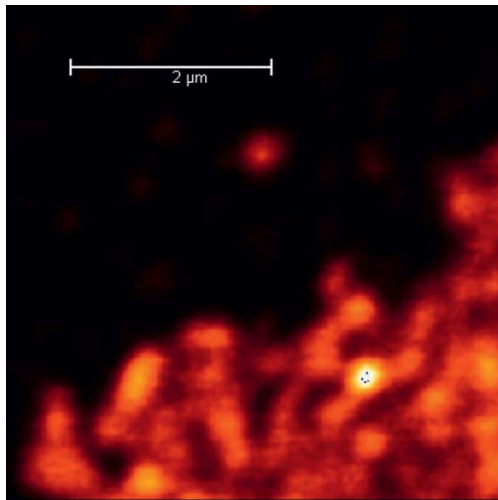

Confocal image

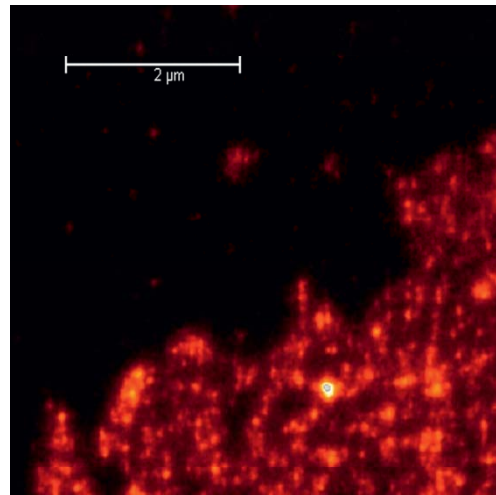


STED image


Images: Prof. Dr. T. Lang, Univ. Of Bonn, germany and Leica Microsystems




# Atomic Force Microscopy (AFM)



- A method to record the topographic property of a surface
- Physical interaction with the surface is necessary

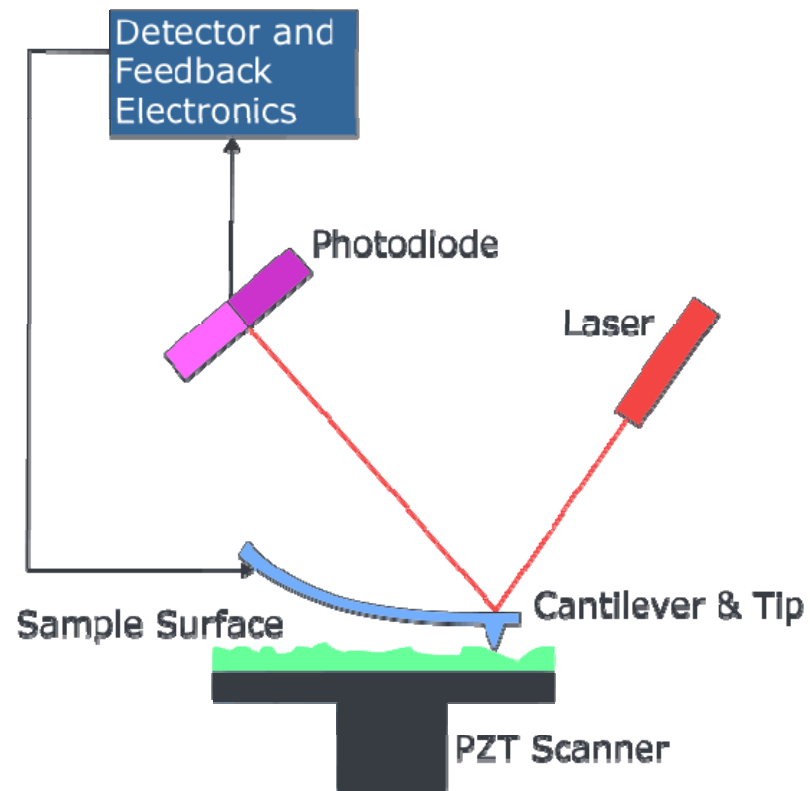

# The principle

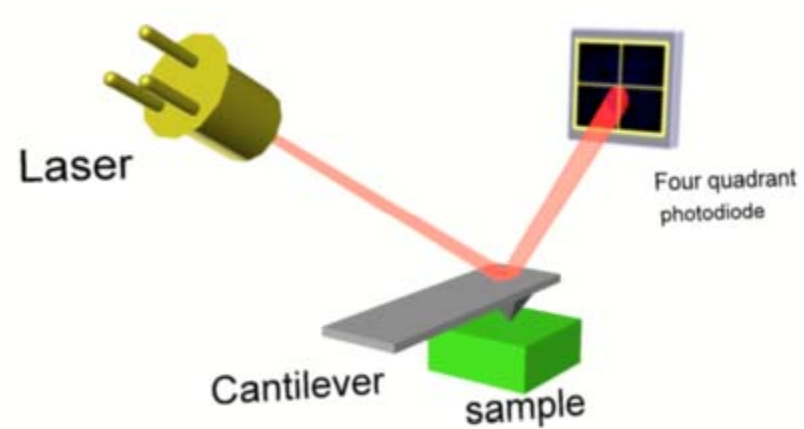

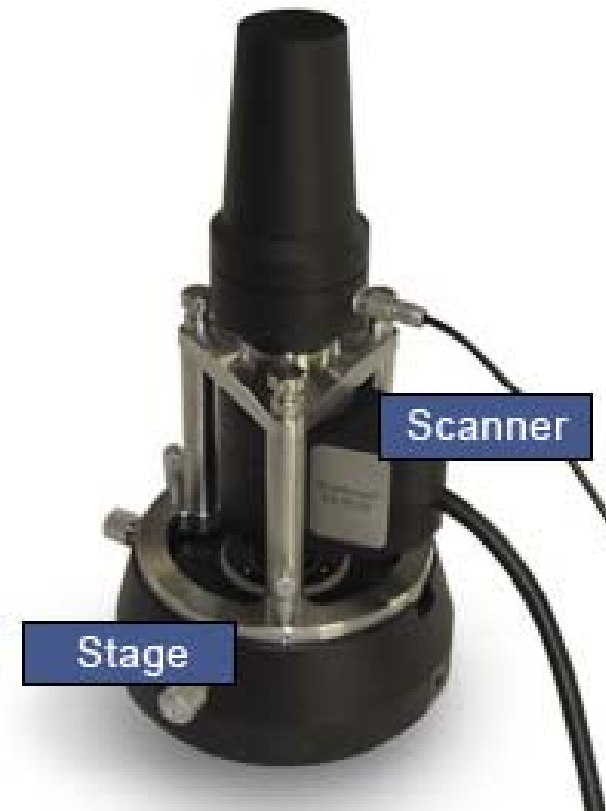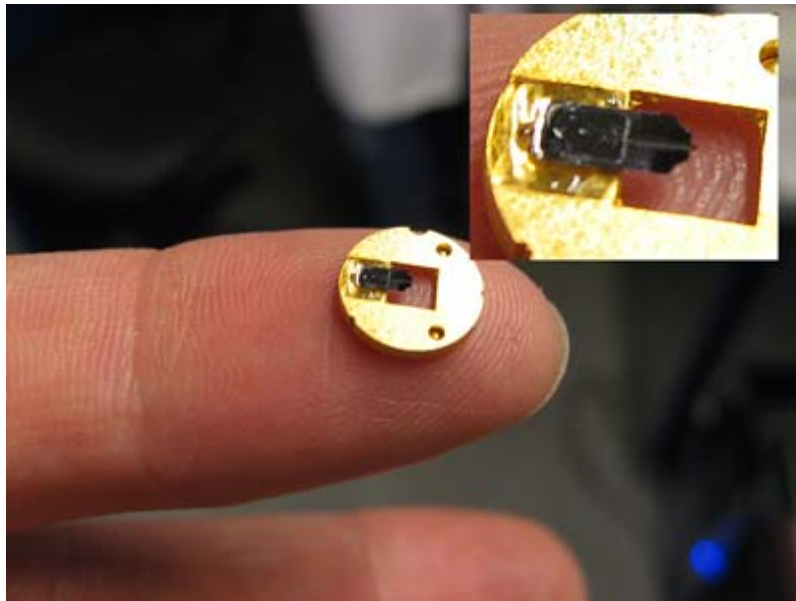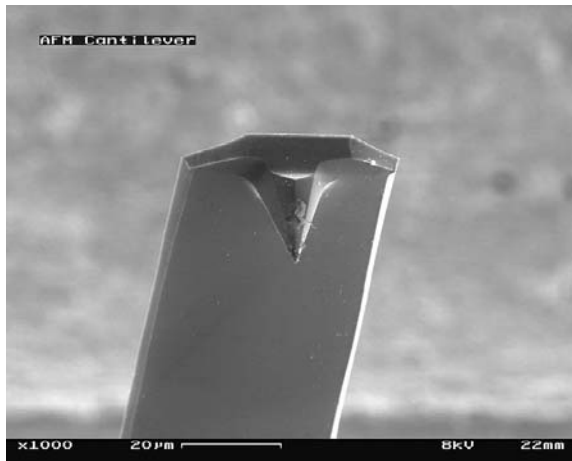

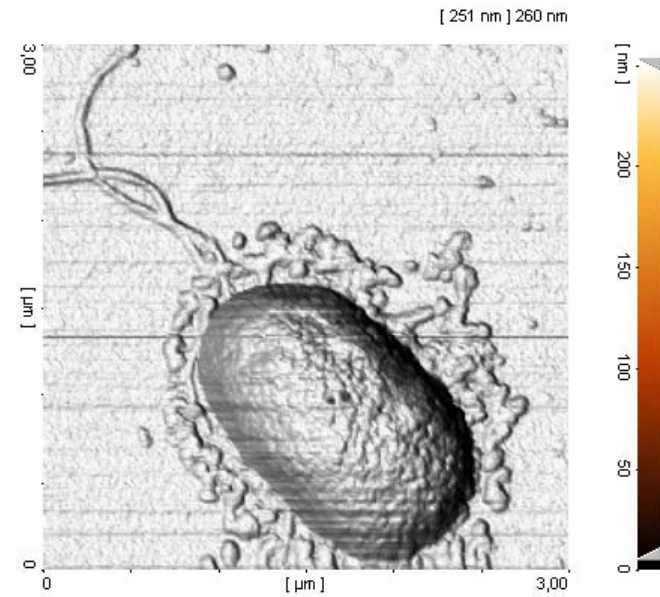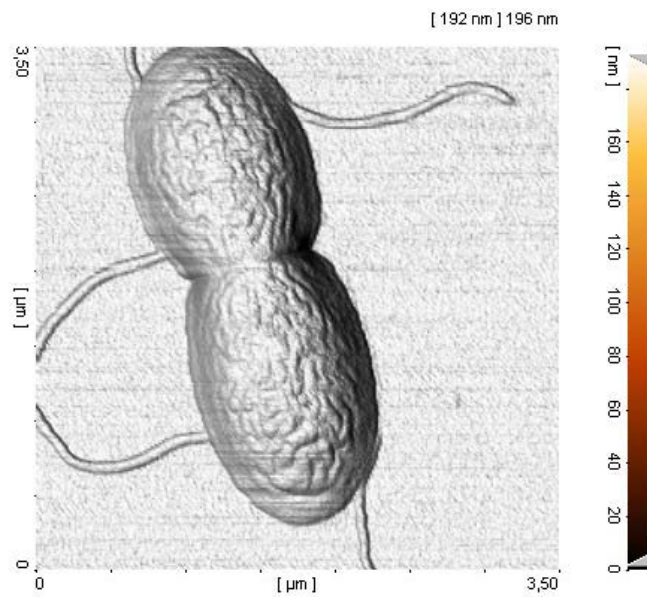

Anne Louise Frost m.fl. 2007 (unpublished)

## Benefits of AFM

- Extremely high resolution (down to atomic level few Å), but typically 10-20 nm)
- No staining required
- Possible to measure attractive/repulsive forces

## Disadvantages of AFM

- Extremely high resolution (very low "focal depth")
- Small image area
- Sample must be "flat" and tightly fixed
- Very difficult to work in humid or wet environments
- Need direct contact to sample
- Imaging depends on tip shape
- Slow

